



# Performance Test Certificate


TEMP/TIME	VOLTAGE	MODEL NUMBER	SERIAL NUMBER
121C/18min	120V	210006AC	10041379

STERILIZING TEMPERATURE (°C)			OPERATING PRESSURE (bar minimum)	MINIMUM HOLD TIME (minutes)	MAXIMUM CYCLE TIME (minutes)
Nominal	Min	Max			
123.0	121.0	125.0	1.05	18.0	28

MAXIMUM DESIGN TEMPERATURE (°C)	THERMAL FUSE CIRCUIT ACTIVATING TEMPERATURE (°C)	SINGLE FAULT MAXIMUM TEMPERATURE (°C) (Please note - this is the maximum temperature to which any load may be subjected following any single fault condition)	PRIMARY SAFETY VALVE RELEASE PRESSURE (bar)	OVER PRESSURE SAFETY DEVICE RELEASE PRESSURE (bar)
131.3	152.0	130.0	1.79	7.00

Maximum permissible load *including chamber furniture* as follows:

3kg

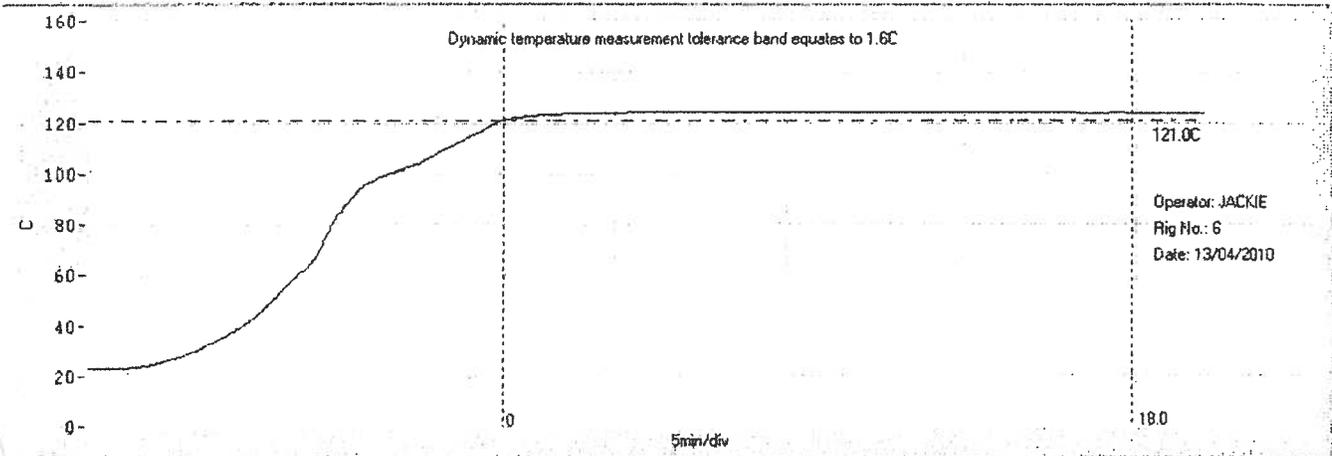

This unique chart recording shows the temperature reached during the automatic final test. This recording pertains to the model and serial number of the Autoclave shown at the top of this certificate, and is not transferable.

**UNIMAX TESTING SERVICES**  
269 Canal St. New York, NY 10013

**Test Results:**  
**PASSED**

**STERILITY ASSURANCE REPORT-  
BIOLOGICAL SPORE TEST RESULTS FOR**

Steve King  
King's Ink  
136 Main St  
Action, MA  
01720

**CERTIFICATE OF  
AUTOCLAVE  
TESTING**

**Your Autoclave Sterilizer PASSED Bio-  
logical Spore Testing**

**Spore test results showed no growth**

**indicating that your sterilization procedures and equipment have**

Test No.	Test Date	Cust. Cycle Date	Autoclave Mfg.	Model	Serial
9753	4/7/11	4/2/11	Prestige Medical	210006AC	10041379

**passed testing.**

**Sterility Assurance Means:**

**Repeated biological testing consistently produces negative results.**

**Unimax Testing Services**

**269 Canal St, 2nd Floor**

**New York, NY 10013**

**212-925-1051**

***Congratulations***



**UNIMAX TESTING SERVICES**  
269 Canal St. New York, NY 10013

**Test Results:**  
**PASSED**

**STERILITY ASSURANCE REPORT-  
BIOLOGICAL SPORE TEST RESULTS FOR**

King'slnk  
136 Main St  
Action, MA  
01720

**CERTIFICATE OF  
AUTOCLAVE  
TESTING**

**Your Autoclave Sterilizer PASSED Bio-  
logical Spore Testing**

**Spore test results showed no growth  
indicating that your sterilization procedures and equipment have**

Test No.	Test Date	Cust. Cycle Date	Autoclave Mfg.	Model	Serial
10025	5/27/11	5/3/11	Prestige Medi- cal	210006AC	10041379

**passed testing.**

**Sterility Assurance Means:**

**Repeated biological testing consistently produces negative results.**

**Unimax Testing Services**  
269 Canal St, 2nd Floor  
New York, NY 10013  
212-925-1051  
*Congratulations*



**UNIMAX TESTING SERVICES**  
269 Canal St. New York, NY 10013

**Test Results:**  
**PASSED**

**STERILITY ASSURANCE REPORT-  
BIOLOGICAL SPORE TEST RESULTS FOR**

King's Ink  
136 Main St  
Action, MA  
01720

**CERTIFICATE OF  
AUTOCLAVE  
TESTING**

Your Autoclave Sterilizer **PASSED** Bio-  
logical Spore Testing

Spore test results showed no growth  
indicating that your sterilization procedures and equipment have

Test No.	Test Date	Cust. Cycle Date	Autoclave Mfg.	Model	Serial
10373	8/10/11	8/4/11	Prestige Medical	210006AC	10041379

passed testing.

**Sterility Assurance Means:**

**Repeated biological testing consistently produces negative results.**

Unimax Testing Services  
269 Canal St, 2nd Floor  
New York, NY 10013  
212-925-1051

*Congratulations*



**UNIMAX TESTING SERVICES**  
269 Canal St. New York, NY 10013

**Test Results:**  
**PASSED**

**STERILITY ASSURANCE REPORT-  
BIOLOGICAL SPORE TEST RESULTS FOR**

King's Ink  
136 Main St  
Action, MA  
01720

**CERTIFICATE OF  
AUTOCLAVE  
TESTING**

**Your Autoclave Sterilizer PASSED Bio-  
logical Spore Testing**

**Spore test results showed no growth  
indicating that your sterilization procedures and equipment have**

Test No.	Test Date	Cust. Cycle Date	Autoclave Mfg.	Model	Serial
10770	10/25/11	10/1/11	Prestige Medical	210006AC	10041379

**passed testing.**

**Sterility Assurance Means:**

**Repeated biological testing consistently produces negative results.**

Unimax Testing Services  
269 Canal St, 2nd Floor  
New York, NY 10013  
212-925-1051

***Congratulations***



**UNIMAX TESTING SERVICES**  
269 Canal St. New York, NY 10013

**Test Results:**  
**PASSED**

**STERILITY ASSURANCE REPORT-  
BIOLOGICAL SPORE TEST RESULTS FOR**

Stephen King  
136 Main St.  
Acton, MA  
01720

**CERTIFICATE OF  
AUTOCLAVE  
TESTING**

**Your Autoclave Sterilizer PASSED  
Biological Spore Testing**

**Spore test results showed no growth  
indicating that your sterilization procedures and equipment have**

Test No.	Test Date	Cust. Cycle Date	Autoclave Mfg.	Model	Serial
11389	3/7/12	3/1/12	Prestige	210006AC	10041379


**passed testing.**

**Sterility Assurance Means:**

**Repeated biological testing consistently produces negative results.**

**Unimax Testing Services  
269 Canal St, 2nd Floor  
New York, NY 10013  
212-925-1051**

***Congratulations***

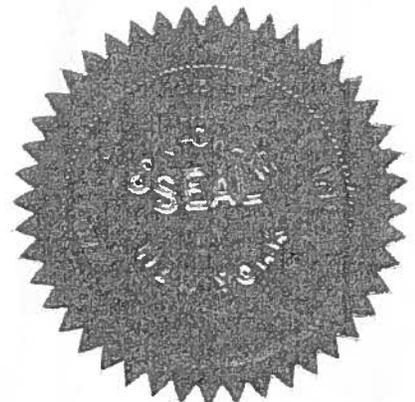

**UNIMAX TESTING SERVICES**  
269 Canal St. New York, NY 10013

**Test Results:**  
**PASSED**

**STERILITY ASSURANCE REPORT-  
BIOLOGICAL SPORE TEST RESULTS FOR**

**Stephen King dba King's Ink**  
136 Main St.  
Acton, MA  
01720

**CERTIFICATE OF  
AUTOCLAVE  
TESTING**

**Your Autoclave Sterilizer PASSED  
Biological Spore Testing**

**Spore test results showed no growth  
indicating that your sterilization procedures and equipment have**

Test No.	Test Date	Cust. Cycle Date	Autoclave Mfg.	Model	Serial
11999	7/9/12	7/3/12	Prestige Medical	210006AC	10041379

**passed testing.**

**Sterility Assurance Means:**

**Repeated biological testing consistently produces negative results.**

**Unimax Testing Services**  
269 Canal St, 2nd Floor  
New York, NY 10013  
212-925-1051

***Congratulations***



**UNIMAX TESTING SERVICES**  
269 Canal St. New York, NY 10013

**Test Results:**  
**PASSED**

**STERILITY ASSURANCE REPORT  
BIOLOGICAL SPORE TEST RESULTS FOR**

King's Ink  
136 Main St.  
Acton, MA 01720

**CERTIFICATE OF  
AUTOCLAVE  
TESTING**

**Your Autoclave Sterilizer PASSED  
Biological Spore Testing**

**Spore test results showed no growth indicating that your  
sterilization procedures and equipment have passed testing.**

**Sterility Assurance Means:**

Test Number	Unimax Test Date	Customer Cycle Date	Autoclave Manufacturer	Model	Serial Number
12158	6/12/13	-	Prestige Medical	210006 AC	10041379

**Repeated biological testing consistently produces negative results.**

**Unimax Testing Services  
269 Canal St, 2nd Floor  
New York, NY 10013  
212-925-1051**

***Congratulations.***



**UNIMAX TESTING SERVICES**  
269 Canal St. New York, NY 10013

**Test Results:**  
**PASSED**

**STERILITY ASSURANCE REPORT  
BIOLOGICAL SPORE TEST RESULTS FOR**

King's Ink  
136 Main St.  
Acton, MA 01720

**CERTIFICATE OF  
AUTOCLAVE  
TESTING**

Your Autoclave Sterilizer **PASSED**  
Biological Spore Testing

Spore test results showed no growth indicating that your sterilization procedures and equipment have passed testing.

Test Number	Unimax Test Date	Customer Cycle Date	Autoclave Manufacturer	Model	Serial Number
12229	7/3/13	6/29/13	Prestige Medical	210006AC	10041379

**Sterility Assurance Means:**  
**Repeated biological testing consistently produces negative results.**

Unimax Testing Services  
269 Canal St, 2nd Floor  
New York, NY 10013  
212-925-1051

*Congratulations.*



**UNIMAX TESTING SERVICES**  
269 Canal St. New York, NY 10013

**Test Results:**  
**PASSED**

**STERILITY ASSURANCE REPORT**  
**BIOLOGICAL SPORE TEST RESULTS FOR**

King's Ink  
136 Main St.  
Acton, MA 01720

**CERTIFICATE OF**  
**AUTOCLAVE**  
**TESTING**

Your Autoclave Sterilizer **PASSED**  
Biological Spore Testing

Spore test results showed no growth indicating that your sterilization procedures and equipment have passed testing.

Test Number	Unimax Test Date	Customer Cycle Date	Autoclave Manufacturer	Model	Serial Number
12777	11/20/13	11/6/13	Prestige Medical	210006AC	10041379

**Sterility Assurance Means:**  
Repeated biological testing consistently produces negative results.

Unimax Testing Services  
269 Canal St, 2nd Floor  
New York, NY 10013  
212-925-1051

*Congratulations.*



**UNIMAX TESTING SERVICES**  
269 Canal St. New York, NY 10013

**Test Results:**  
**PASSED**

**STERILITY ASSURANCE REPORT  
BIOLOGICAL SPORE TEST RESULTS FOR**

King's Ink  
136 Main St.  
Acton, MA 01720

**CERTIFICATE OF  
AUTOCLAVE  
TESTING**

Your Autoclave Sterilizer PASSED  
Biological Spore Testing

Spore test results showed no growth indicating that your  
sterilization procedures and equipment have passed testing.

Test Number	Unimax Test Date	Customer Cycle Date	Autoclave Manufacturer	Model	Serial Number
12892	12/26/13	12/3/13	Prestige Medical	210006AC	10041379

**Sterility Assurance Means:**  
Repeated biological testing consistently produces negative results.

Unimax Testing Services  
269 Canal St, 2nd Floor  
New York, NY 10013  
212-925-1051

*Congratulations.*



**UNIMAX TESTING SERVICES**  
269 Canal St. New York, NY 10013

**Test Results:**  
**PASSED**

**STERILITY ASSURANCE REPORT**  
**BIOLOGICAL SPORE TEST RESULTS FOR**

King's Ink  
136 Main St.  
Acton, MA 01720

**CERTIFICATE OF**  
**AUTOClave**  
**TESTING**

Your Autoclave Sterilizer **PASSED**  
Biological Spore Testing

Spore test results showed no growth indicating that your  
sterilization procedures and equipment have passed testing.

Test Number	Unimax Test Date	Customer Cycle Date	Autoclave Manufacturer	Model	Serial Number
13137	2/27/14	1/4/14	Prestige Medical	210006AC	10041379

**Sterility Assurance Means:**  
Repeated biological testing consistently produces negative results.

Unimax Testing Services  
269 Canal St, 2nd Floor  
New York, NY 10013  
212-925-1051

*Congratulations.*



**UNIMAX TESTING SERVICES**  
269 Canal St. New York, NY 10013

**Test Results:**  
**PASSED**

**STERILITY ASSURANCE REPORT**  
**BIOLOGICAL SPORE TEST RESULTS FOR**

**King's Ink**  
136 Main St.  
Acton, MA 01720

**CERTIFICATE OF**  
**AUTOCLAVE**  
**TESTING**

Your Autoclave Sterilizer **PASSED**  
Biological Spore Testing

Spore test results showed no growth indicating that your  
sterilization procedures and equipment have passed testing.

Test Number	Unimax Test Date	Customer Cycle Date	Autoclave Manufacturer	Model	Serial Number
13178	3/5/14	2/27/14	Prestige Medical	210006AC	10041379

**Sterility Assurance Means:**  
Repeated biological testing consistently produces negative results.

Unimax Testing Services  
269 Canal St, 2nd Floor  
New York, NY 10013  
212-925-1051

*Congratulations.*



**UNIMAX TESTING SERVICES**  
269 Canal St. New York, NY 10013

**Test Results:**  
**PASSED**

**STERILITY ASSURANCE REPORT**  
**BIOLOGICAL SPORE TEST RESULTS FOR**

King's Ink  
136 Main St.  
Acton, MA 01720

**CERTIFICATE OF**  
**AUTOCCLAVE**  
**TESTING**

**Your Autoclave Sterilizer PASSED**  
**Biological Spore Testing**

**Spore test results showed no growth indicating that your sterilization procedures and equipment have passed testing.**

Test Number	Unimax Test Date	Customer Cycle Date	Autoclave Manufacturer	Model	Serial Number
13652	7/14/14	7/3/14	Prestige Medical	210006AC	10041379

**Sterility Assurance Means:**  
**Repeated biological testing consistently produces negative results.**

**Unimax Testing Services**  
269 Canal St, 2nd Floor  
New York, NY 10013  
212-925-1051

***Congratulations.***



**UNIMAX TESTING SERVICES**  
269 Canal St. New York, NY 10013

**Test Results:**  
**PASSED**

**STERILITY ASSURANCE REPORT  
BIOLOGICAL SPORE TEST RESULTS FOR**

**King's Ink**  
136 Main St.  
Acton, MA 01720

**CERTIFICATE OF  
AUTOCLAVE  
TESTING**

**Your Autoclave Sterilizer PASSED  
Biological Spore Testing**

**Spore test results showed no growth indicating that your  
sterilization procedures and equipment have passed testing.**

Test Number	Unimax Test Date	Customer Cycle Date	Autoclave Manufacturer	Model	Serial Number
13828	9/6/14	9/2/14	Prestige Medical	210006AC	10041379

**Sterility Assurance Means:  
Repeated biological testing consistently produces negative results.**

**Unimax Testing Services**  
269 Canal St, 2nd Floor  
New York, NY 10013  
212-925-1051

***Congratulations.***



**UNIMAX TESTING SERVICES**  
269 Canal St. New York, NY 10013

**Test Results:**  
**PASSED**

**STERILITY ASSURANCE REPORT**  
**BIOLOGICAL SPORE TEST RESULTS FOR**

**King's Ink**  
136 Main St.  
Acton, MA 01720

**CERTIFICATE OF**  
**AUTOCLAVE**  
**TESTING**

**Your Autoclave Sterilizer PASSED**  
**Biological Spore Testing**

**Spore test results showed no growth indicating that your sterilization procedures and equipment have passed testing.**

Test Number	Unimax Test Date	Customer Cycle Date	Autoclave Manufacturer	Model	Serial Number
14275	1/12/15	1/2/15	Prestige	210006AC	10041379

**Sterility Assurance Means:**  
**Repeated biological testing consistently produces negative results.**

**Unimax Testing Services**  
269 Canal St, 2nd Floor  
New York, NY 10013  
212-925-1051



**UNIMAX TESTING SERVICES**  
269 Canal St. New York, NY 10013

**Test Results:**  
**PASSED**

**STERILITY ASSURANCE REPORT**  
**BIOLOGICAL SPORE TEST RESULTS FOR**

**King's Ink**  
136 Main St.  
Acton, MA 01720

**CERTIFICATE OF**  
**AUTOCLAVE**  
**TESTING**

**Your Autoclave Sterilizer PASSED**  
**Biological Spore Testing**

**Spore test results showed no growth indicating that your sterilization procedures and equipment have passed testing.**

Test Number	Unimax Test Date	Customer Cycle Date	Autoclave Manufacturer	Model	Serial Number
14587	4/6/15	4/1/15	Prestige Medical	210006 AC	10041379

**Sterility Assurance Means:**  
**Repeated biological testing consistently produces negative results.**

**Unimax Testing Services**  
269 Canal St, 2nd Floor  
New York, NY 10013  
212-925-1051

